



# USER MANUAL

## **MS5410**

Chair Scale


















 **PROGRESS HEALTHCARE**  
Caring for you since 1968  
345 Jalan Besar Singapore 208987  
Tel 6297 5955 | [www.progress.com.sg](http://www.progress.com.sg)



Please keep the instruction manual at hand all the time for future reference.

## Explanation of Graphic Symbols on Label/Packaging

|   |   |   |  |
|---|---|---|--|
|    | <p>Caution, consult accompanying documents before use</p>   |    | <p>Separate collection for waste of electrical and electronic equipment, in accordance with Directive 2002/96/EC</p> |
|    | <p>Manufacturer of medical device</p>   |    | <p>Manufacturing year of medical device</p>  |
|    | <p>Carefully read user manual before installation and usage, and follow instructions for use.</p> |    | <p>Medical electrical equipment with Type B applied part</p>   |
|    | <p>Device catalogue number</p>  |    | <p>Authorized representative in the European Community</p>   |
|     | <p>Manufacturer's batch or lot number</p>   |    | <p>Device is a medical device</p>  |
|     | <p>Serial number</p>  |    | <p>Unique Device Identifier</p>  |
|    |   | <p>Device conforms to 93/42/EEC as amended by 2007/47/EC Medical Device Directive. Four digit number refers to Notified Body.</p>   |  |
|   |   | <p>Device complies with International Organization of Legal Metrology (Class III) requirements (verified models only)</p>   |  |
|  |   | <p>Device complies with EC directives (verified models only)</p> <p><b>M</b>: Conformity label in compliance with Directive 2014/31/EU for non-automatic weighing instruments</p> <p><b>18</b>: Year in which conformity verification was performed and the CE label was applied. (ex: 18=2018)</p> <p><b>0122</b>: Refers to Notified Body for metrology</p> |  |

---

## **Copyright Notice**

### **Charder Electronic Co., Ltd.**

No.103, Guozhong Rd., Dali Dist., Taichung City 41262 Taiwan

Tel: +886-4-2406 3766

Fax: +886-4-2406 5612

Website: [www.chardermedical.com](http://www.chardermedical.com) E-mail: [info\\_cec@charder.com.tw](mailto:info_cec@charder.com.tw)

Copyright© Charder Electronic Co., Ltd. All rights reserved.

This user manual is protected by international copyright law. All content is licensed, and usage is subject to written authorization from Charder Electronic Co., Ltd. (hereinafter Charder) Charder is not liable for any damage caused by a failure to adhere to requirements stated in this manual. Charder reserves the right to correct misprints in the manual without prior notice, and modify the exterior of the device for quality purposes without customer consent.



Charder Electronic Co., Ltd.  
No. 103, Guozhong Rd., Dali Dist.,  
Taichung City, 41262 Taiwan

# CONTENTS

|  |           |
|--|-----------|
| <b>I. Safety Notes</b> .....                         | <b>5</b>  |
| A. General Information .....                         | 5         |
| B. EMC Guidance and Manufacturer's Declaration ..... | 8         |
| <b>II. Installation</b> .....                        | <b>12</b> |
| A. Adjusting footrests .....                         | 12        |
| B. Adjusting wheel height .....                      | 14        |
| C. Inserting Batteries .....                         | 15        |
| D. Using Adapter .....                               | 18        |
| <b>III. Indicator</b> .....                          | <b>19</b> |
| A. Indicator and Key Functions .....                 | 19        |
| B. Display layout .....                              | 20        |
| <b>IV. Using Device</b> .....                        | <b>21</b> |
| A. Basic Operation .....                             | 21        |
| B. Hold .....  | 21        |
| C. BMI .....   | 21        |
| D. Tare .....  | 22        |
| E. Pre-Tare .....                                    | 22        |
| F. Print .....                                       | 26        |
| <b>V. Device Setup</b> .....                         | <b>27</b> |
| A. Setting Time & Date .....                         | 27        |
| B. Device Setup .....                                | 28        |
| <b>VI. Setup USB Connection to PC</b> .....          | <b>30</b> |
| <b>VII. Wireless Connection</b> .....                | <b>33</b> |
| <b>VIII. Troubleshooting</b> .....                   | <b>34</b> |
| <b>IX. Product Specifications</b> .....              | <b>36</b> |
| <b>X. Declaration of Conformity</b> .....            | <b>40</b> |



## I. Safety Notes

### A. General Information

Thank you for choosing this Charder Medical device. It is designed to be easy and straightforward to operate, but if you encounter any problems not addressed in this manual, please contact your local Charder service partner.

Before beginning operation of the device, please read this user manual carefully, and keep it in a safe place for reference. It contains important instructions regarding installation, proper usage, and maintenance.

### Intended Use

This device is intended to measure the weight of subjects with limited mobility, for diagnosis of weight-related issues by professionals.

### General Handling

- Device should be placed on stable, flat, solid, non-slippery surface.
- Usage on soft surfaces (ex: carpet) may result in inaccurate results.
- Ensure all parts are properly locked and tightened before operating the device.
- Device is intended to measure one subject at a time.

### Safety Instructions

- Batteries should be kept away from children. If swallowed, promptly seek medical assistance.
- Expected service life: 5 years.
- Always comply with appropriate regulations when using electrical components under increased safety requirements.
- Ensure voltage marked on power supply matches mains power supply.
- The device is intended for indoor use only.
- Observe permissible ambient temperatures for use

### Environmental

- All batteries contain toxic compounds; batteries should be disposed of via designated competent organizations. Batteries should not be incinerated.

### Cleaning

- Device surface should be cleaned using alcohol-based wipes. Corrosive cleansing liquids should not be used. Pressure-washers should not be used.

- Do not use large amounts of water when cleaning the device, as it may cause damage to the internal electronics.
- Always disconnect device from mains power before cleaning.

## **Maintenance**

- Device does not require routine maintenance. However, regular checking of accuracy is recommended; frequency to be determined by level of use and state of device. If results are inaccurate, please contact local distributor.

## **Warranty/Liability**

- The period of warranty shall be eighteen (18) months, beginning on the date of purchase. Please retain your receipt as proof of purchase.
- No responsibility shall be accepted for damage caused through any of the following reasons: unsuitable or improper storage or use, incorrect installation or commissioning by the owner or third parties, natural wear and tear, changes or modifications, incorrect or negligent handling, chemical, electrochemical, or electrical interference.
- All maintenance, technical inspections, and repairs should be conducted by an authorized Charder service partner, using original Charder accessories and spare parts. Charder is not liable for any damages arising from improper maintenance or usage.

## **Disposal**

- This product is not to be treated as regular household waste, but should be taken to a designated collection points for electronics. Further information should be provided by local waste disposal authorities.



## **Warning**

- Only the original adapter should be used with the device. Using an adapter other than the one provided by Charder may cause malfunction.
- Do not touch the power supply with wet hands.
- Do not crimp the power cable, and avoid sharp edges.
- Do not overload extension cables connected to the device.
- Route cables carefully, to avoid tripping.
- Keep device away from liquids.
- Do not remove the plug by yanking on the cable.
- Use only a correctly wired (100-240VAC) outlet, and do not use a multiple outlet extension cable.

- Do not under any circumstances dismantle or alter the device, as this could result in electric shock or injury as well as adversely affect the precision of measurements.
- Do not place the device in direct sunlight, or in close proximity to an intense heat source. Excessively high temperatures may damage the internal electronics.



### **Warning**

Measurements for physically disabled persons.

- Physically disabled persons should not attempt to take measurements alone, but instead should have their caretakers assist them in using the device.
- Footrest can only be used when subject is sitting in chair. To avoid injury, subject should refrain from standing on footrest, as device may tip over if used incorrectly.



### **Incident Reporting**

Any serious incident that has occurred in relation to the device should be reported to the manufacturer, EU representative (if device is used in EU member state), and competent authority of user/subject's member state.

## B. EMC Guidance and Manufacturer's Declaration

| <b>Guidance and manufacturer's declaration-electromagnetic emissions</b>   |                   |   |
|--|-------------------|---|
| <p>The MS5410 Chair Scale is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.</p> |                   |   |
| <b>Emission test</b>   | <b>Compliance</b> | <b>Electromagnetic environment-guidance</b>   |
| RF emissions CISPR 11  | Group 1           | The device uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.   |
| RF emissions CISPR 11  | Class B           | The device is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes. |
| Harmonic emissions IEC 61000-3-2   | Class A           |   |
| Voltage fluctuations /flicker emissions IEC 61000-3-3  | Compliance        |   |




### Guidance and manufacturer's declaration-electromagnetic immunity

The MS5410 Chair Scale is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.

| Immunity test  | IEC 60601 test level   | Compliance level   | Electromagnetic environment-guidance   |
|--|--|--|--|
| Electrostatic discharge(ESD)<br>IEC 61000-4-2  | <u>± 8 kV contact</u><br><u>± 2 kV, ± 4 kV,</u><br><u>± 8 kV, ± 15 kV</u><br><u>air</u>  | <u>± 8 kV contact</u><br><u>± 2 kV, ± 4 kV,</u><br><u>± 8 kV, ± 15 kV</u><br><u>air</u>  | Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%   |
| Electrical fast transient/burst<br>IEC 61000-4-4   | ± 2kV for power supply lines<br>+ 1kV for input/output lines   | + 2kV for power supply lines<br>+ 1kV for input/output lines   | Mains power quality should be that of a typical commercial or hospital environment.  |
| Surge IEC<br>61000-4-5   | ± 1kV line(s) to line(s)<br>± 2kV line(s) to earth   | + 1kV line(s) to line(s)<br>+ 2kV line(s) to earth   | Mains power quality should be that of a typical commercial or hospital environment.  |
| Voltage Dips, short interruptions and voltage variations on power supply input lines IEC<br>61000-4-11 | <u>0% UT for 0,5 cycle</u><br><u>0% UT for 1 cycle</u><br><br><u>70% UT(30% dip in UT) for 25 cycles</u><br><br><u>0% UT for 5 s</u> | <u>0% UT for 0,5 cycle</u><br><u>0% UT for 1 cycle</u><br><br><u>70% UT(30% dip in UT) for 25 cycles</u><br><br><u>0% UT for 5 s</u> | Mains power quality should be that of a typical commercial or hospital environment. If the user of the device requires continued operation during power mains interruptions, it is recommended that the device be powered from an uninterruptible power supply or a battery. |
| Power frequency(50/60 Hz) magnetic field<br>IEC 61000-4-8  | <u>30 A/m</u>  | <u>30 A/m</u>  | The device power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.   |
| NOTE UT is the a.c. mains voltage prior to application of the test level.                              |  |  |  |

### Guidance and manufacturer's declaration-electromagnetic immunity

The MS5410 Chair Scale is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that is used in such an environment.

| Immunity test  | IEC 60601 test level   | Compliance level  | Electromagnetic environment-guidance   |
|--|--|---|--|
| <p>Conducted RF IEC 61000-4-6</p> <p>Radiated RF IEC 61000-4-3</p> | <p>3 Vrms<br/>150 KHz to 80 MHz</p> <p><u>6 V in ISM bands between 0,15 MHz and 80 MHz</u><br/><u>80 % AM at 1 kHz</u></p> <p>3 V/m<br/>80MHz to 2,7 GHz</p> | <p>3 Vrms<br/>150 KHz to 80 MHz</p> <p><u>6 V in ISM bands between 0,15 MHz and 80 MHz</u><br/><u>80 % AM at 1 kHz</u></p> <p>3 V/m<br/><u>80MHz to 2,7 GHz</u></p> | <p>Portable and mobile RF communications equipment should be used no closer to any part of the device including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p><b>Recommended separation distance:</b><br/> <math>d = 1,2 \sqrt{P}</math><br/> <math>d = 1,2 \sqrt{P}</math> 80MHz to 800 MHz<br/> <math>d = 2,3 \sqrt{P}</math> 800MHz to 2,5 GHz</p> <p>Where <math>P</math> is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and <math>d</math> is the recommended separation distance in metres (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey<sup>a</sup>, should be less than the compliance level in each frequency range<sup>b</sup>.</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> <div style="text-align: center;">  </div> |

NOTE1 At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

- a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the device is used exceeds the applicable RF compliance level above, the device should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the device.
- b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

**Recommended separation distance between portable and mobile RF communications equipment and the MS5410 Chair Scale**

The device is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the device can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the device as recommended below, according to the maximum output power of the communications equipment.

| Rated maximum output power of transmitter<br><br>W | Separation distance according to frequency of transmitter m |  |   |
|--|---|--|---|
|  | 150 kHz to 80 MHz<br>$d = 1,2\sqrt{P}$                      | 80 MHz to 800 MHz<br>$d = 1,2\sqrt{P}$ | 800 MHz to 2,5 GHz<br>$d = 2,3\sqrt{P}$ |
| 0,01   | 0,12  | 0,12                                   | 0,23                                    |
| 0,1  | 0,38  | 0,38                                   | 0,73                                    |
| 1  | 1,2   | 1,2                                    | 2,3                                     |
| 10   | 3,8   | 3,8                                    | 7,3                                     |
| 100  | 12  | 12                                     | 23                                      |

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $p$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.


## II. Installation

### A. Adjusting footrests


1. Remove bolt to adjust length of footrest



2. Adjust footrest height according patient leg length

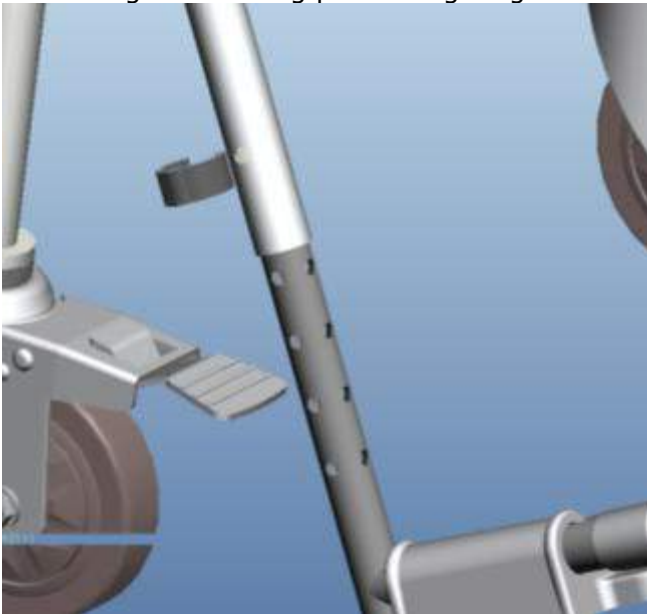

3. After completing adjustment, insert bolts to secure footrest

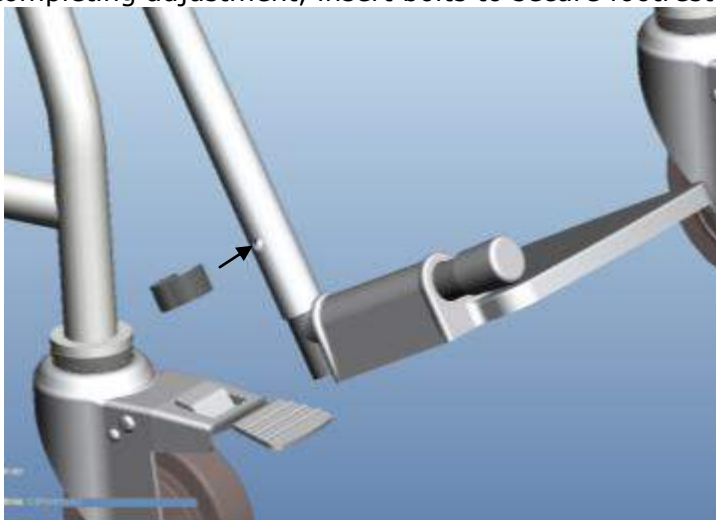

## B. Adjusting wheel height

1. Place device on flat surface, apply wheel brakes



Brakes

2. To tighten wheel castor, loosen counternut slightly. After loosening, turn wheel frame clockwise to tighten.



Counternut

Wheel frame


3. Adjust wheel height until air bubble on level indicator is level





**NOTE:** Be careful not to lose wheels during adjustment

## C. Inserting Batteries


1. Open battery housing cover

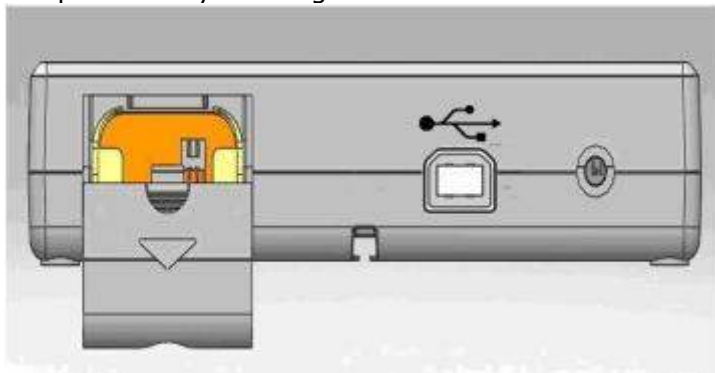


2. Accessing batteries

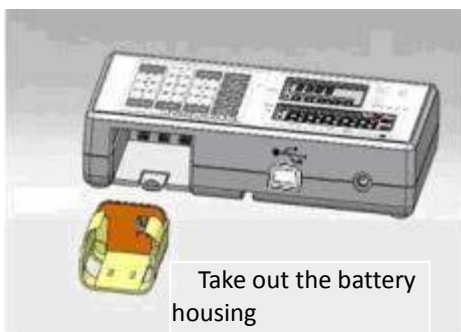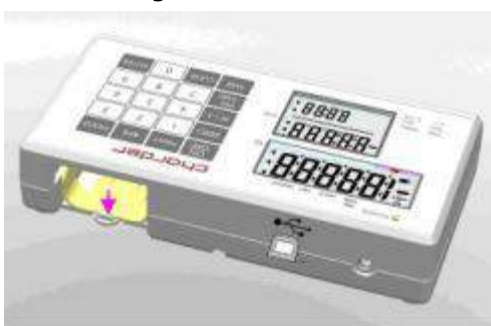


3. Use either rechargeable battery pack, or AA batteries

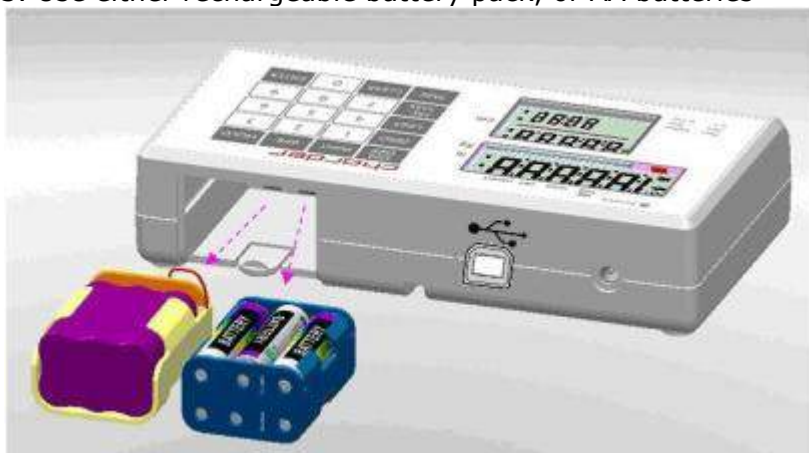

4. Ensure batteries are installed into the housing correctly

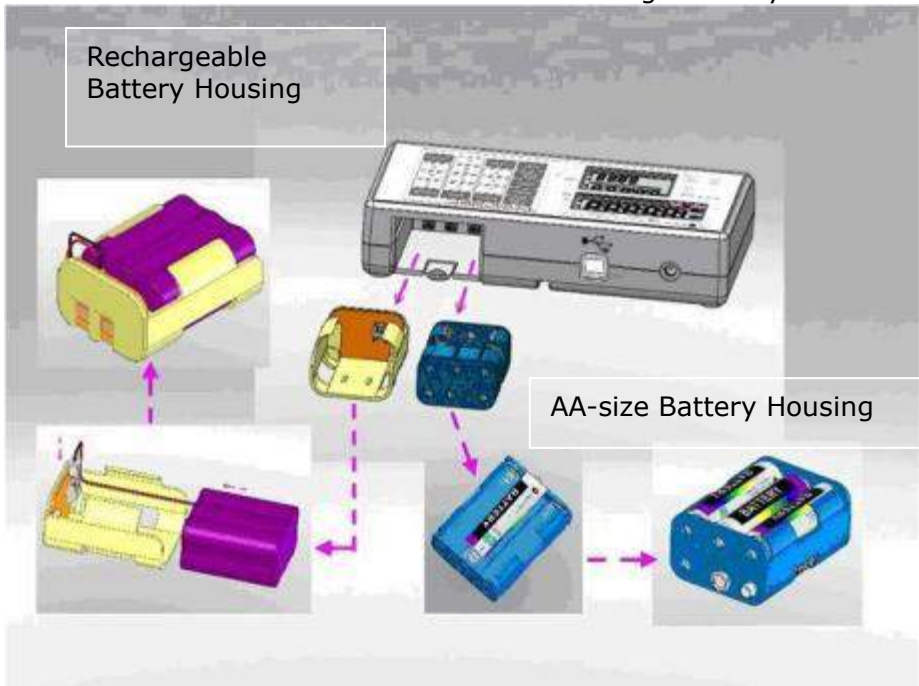


5. Install the battery housing into the compartment, and make sure the right side of housing pin is facing towards inside of the connecting position

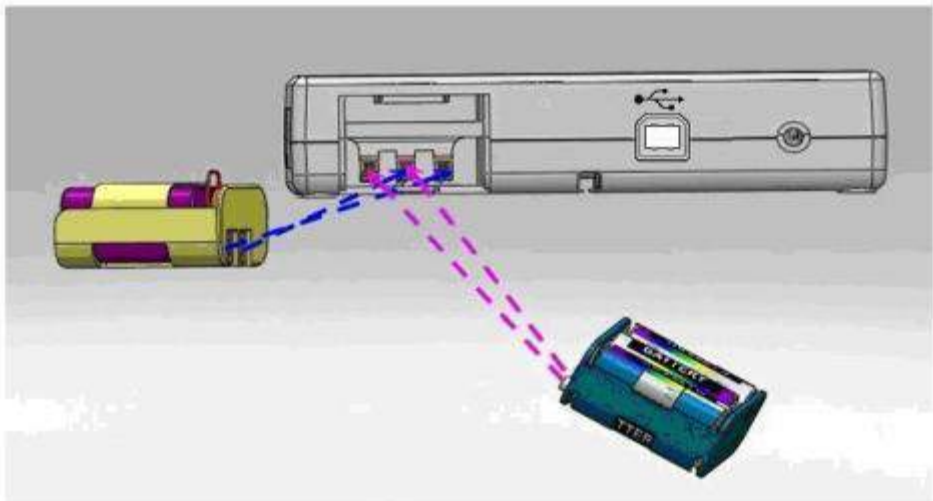



6. Slide back the cover to close the battery housing compartment. Turn on power to confirm that battery is correctly installed.

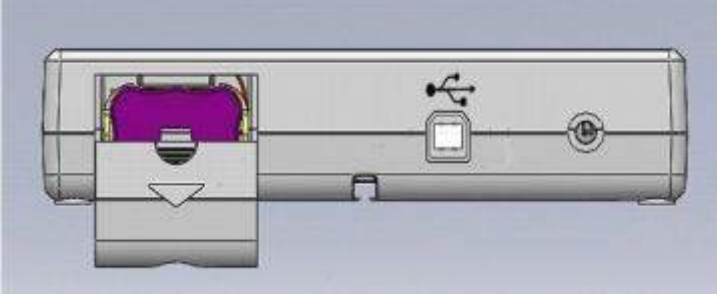


### Using Rechargeable Battery (optional)

The rechargeable battery should be recharged at least once every 3 months, regardless of if the device has been used. Battery can be charged by plugging device's exclusive adapter into AC Connector Port.

After a long period in storage (e.g. >3 months), the battery should run a full cycle (charge/discharge) to allow it to restore full capacity.


Ensure rechargeable battery housing is installed and inserted properly into the compartment.

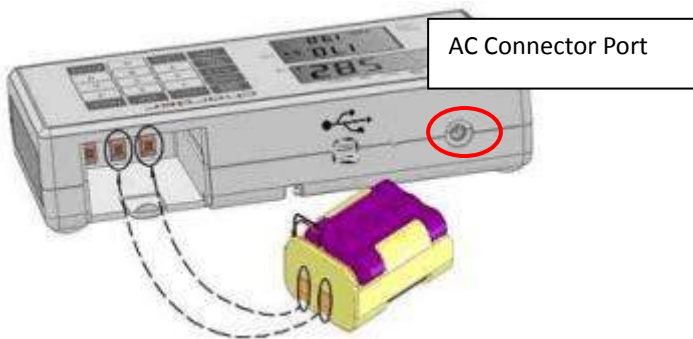

If Lo prompt displays on the LCD, please charge battery promptly to avoid battery damage.

## D. Using Adapter

1. Connect adapter to indicator before connecting to mains power supply
2. Disconnect adapter from mains power supply before unplugging adapter pin from indicator.

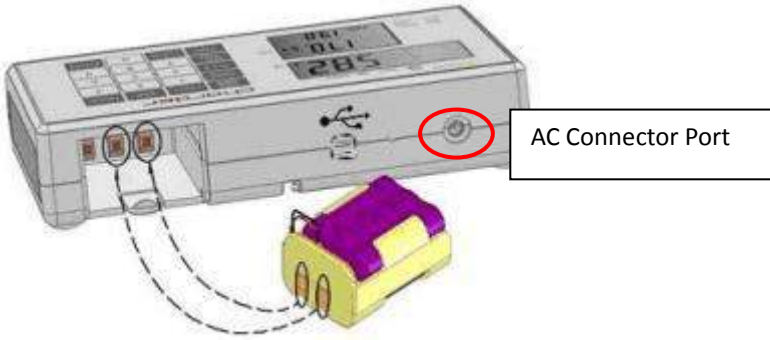










# III. Indicator

## A. Indicator and Key Functions




(Wireless functionality optional)

### Key Function

-  **ON/OFF**: Power on or power off.
-  **ZERO**: Reset display to 0.0 kg display. Press and hold for 3 seconds to enter device settings.
-  **M1-5**: Saving pre-tare values (up to 5)
-  **PRE-TARE**: Pre-tare the known weight of an object (ex: chair) before beginning measurement.
-  **TARE**: Allows user to deduct weight from reading after measurement
-  **PRINT**: When printer or PC is connected to the scale, press this key to print results
-  **BMI**: Calculation of Body Mass Index
-  **HOLD**: Determine stable weighing value - used when weight is unstable. Press and hold for 3 seconds to enter time setting.
-  **0-9**: For entering digits.

10. **CLEAR**: Clear incorrect data input.
11. **ENTER**: Confirm input

## B. Display layout

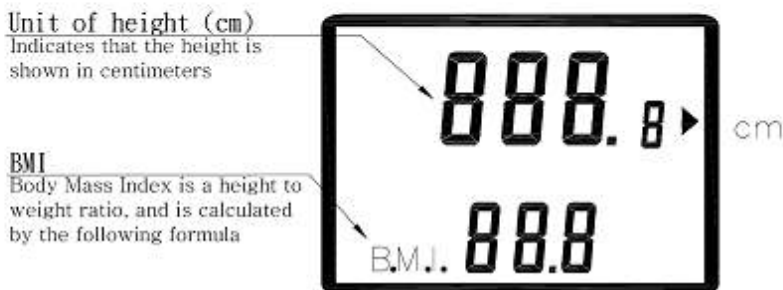

## Definitions

**Stable symbol:** Indicate that weight is stable.

**Zero symbol:** Weight is at zero

**Negative weight:** Weight under zero.


**Low battery:** Battery needs to be charged or replaced.

## IV. Using Device

### A. Basic Operation

Switch on the device using  key. The device will automatically perform self-calibration, displaying software version.

Once "0.00 kg" appears on indicator, device is ready for measurement.

**Note:** If "0.00 kg" does not display on indicator, press  key to zero the device.



Guide subject to sit on chair. Make sure subject's feet are off the ground, and properly placed upon footrests. After the weight has stabilized, the "stable" symbol will appear on indicator.

**Note:** If subject's weight exceeds scale capacity, indicator will display "Err" prompt due to overload.

### B. Hold

The hold function determines average weight, designed to be used if subject's weight will not stabilize (ex: an active child).




**Note:** if fluctuation is too severe, average weight determination will be difficult and hold may not function correctly

1. Switch on the device normally.
2. Press the  key. "HOLD" will be displayed on the indicator.
3. Guide subject to sit on chair.
4. After a few seconds, the average weight will be displayed on the indicator. This weight will be locked - at this point, subject can stand up from chair.
5. To release the locked weight, press the  key again to return to the device to normal mode.


**Note:** Hold function can be activated before or after subject sits in chair. However, if subject finds it difficult to sit still, we recommend activating Hold after subject is seated.

### C. BMI

1. In normal mode, press the  key to enter BMI mode.

2. Display will show last recorded height. Left-most digit will flash.
3. Enter height using numeral keys (ex: 170 cm). Input will automatically move to next digit. Press  key to re-input. Press  key to manually move to next digit.
4. After inputting height, press  to confirm.
5. Proceed to weigh subject as usual. Indicator will display weight, height, and BMI.

**NOTE:** Hold function can be used at this time if weight is unstable



6. Press  key to return to normal mode.

| Category  | BMI (kg/m <sup>2</sup> ) | Risk of obesity-related disease |
|-----------|--------------------------|---------------------------------|
| Under     | < 18.5                   | Low                             |
| Normal    | 18.5-24.9                | Average                         |
| Over      | 24.9-29.9                | Slightly Increased              |
| Obese I   | 30.0-34.9                | Increased                       |
| Obese II  | 35.0-39.9                | High                            |
| Obese III | > 40                     | Very High                       |

(World Health Organization adult BMI standards)

#### D. Tare


The tare function allows the user to deduct the weight of objects from the device's measurement result.

1. Place object that needs to be tared onto measurement platform.
2. Press  key after stable symbol appears on indicator. Display will indicate "0.00 kg".
3. Guide subject (plus tared object) to sit in chair. Conduct measurement.
4. To clear tare value, remove all objects from measurement platform, and press  key.






#### E. Pre-Tare

The Pre-Tare function is used to subtract the known weight of a substance prior to weighing. The device can store 5 sets of pre-tare values.









Pre-tare values can be stored using two different methods: "Load Weight", or "Input Manually".

After pre-tare weights have been stored, they can be recalled by holding the  key for 3 seconds.

### A. Load Weight

| DESCRIPTION  | EXAMPLE   |
|--|---|
| <p>Press  key after loading weight on the platform; the indicator will display blinking "m" symbol.</p> |   |
| <p>Press numeral key 1 ~ 5 to assign this number with the current pre-tare weight.</p>   |   |
| <p>Press  key to store pre-tare weight; the indicator will make a beep sound.</p>                     |  |


## B. Input Manually

| DESCRIPTION  | EXAMPLE  |
|--|--|
| <p>Press  key. Left-most digit will begin blinking.</p> <p>If no further action is taken within 6 seconds, indicator will return to normal mode</p> |    |
| <p>While digit is blinking:</p> <p>Enter pre-tare weight using 0~9 keys.</p> <p>Ex: to pre-tare 5.0 kg of weight, press 0-0-5-0.</p> <p>Ex: to pre-tare 13.5 kg of weight, press 0-1-3-5.</p>  |    |
| <p>Press  key to confirm the pre-tare weight.</p>   |   |
| <p>Indicator will display minus sign to the left of pre-tare weight value.</p>   |  |
| <p><b>To save this pre-tare weight value in memory:</b></p> <p>Press  key; the blinking "m" symbol will appear on the display.</p>                |  |



Press numeral key 1 ~ 5 to assign this number with the current pre-tare weight.




Press  key to store pre-tare weight; the indicator will make a beep sound.



### C. Recall Pre-Tare Weight


#### DESCRIPTION

#### EXAMPLE

Press and hold  key for 3 seconds. Indicator will display pre-tare value M1 first. The pre-tare value will flash.



**Press numeral keys 1 ~ 5 to choose pre-tare value**

Press  key to confirm which pre-tare weight to select; the device will automatically deduct pre-tare weight.




Press **CLEAR** key to return to Normal Mode



**NOTE:** Pre-tare weight must be under max capacity, otherwise screen will show 0.00 after **ENTER** key is pressed, and the operator will have to re-input pre-tare settings.

## F. Print

If thermal printer is connected to indicator, results can be printed by pressing **PRINT** key.

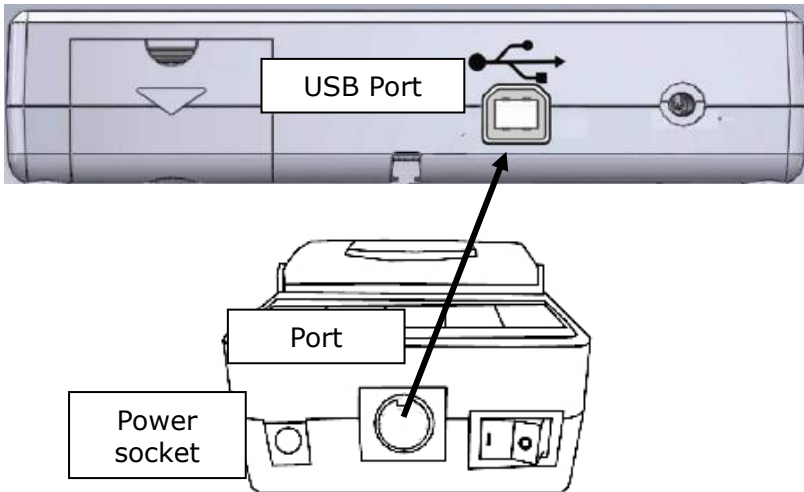









**NOTE:** Thermal printer needs to be powered by adapter

## V. Device Setup


### A. Setting Time & Date

Press and hold  key for 3 seconds to enter Time Setting mode.

Example: Inputting 2008, Dec 25, 8:00am

|  |  |
|--|--|
|   | <p><b>Year Setting</b><br/>Enter year using numeral keys 0-9.</p> <p>Press  key once completed to proceed to month &amp; date setting.</p>  |
|   | <p><b>Month &amp; Day Setting.</b><br/>Enter month, followed by day using numeral keys 0-9.</p> <p>Ex: December 25th is "12.25".<br/>Input 1-2-2-5.</p> <p>Press  key once completed to proceed to time setting.</p>      |
|  | <p><b>Time Setting</b><br/>Enter time (24hr format) using numeral keys 0-9.</p> <p>Ex: 08:00am is input by pressing 0-8-0-0.</p> <p>Press  key once completed to confirm time settings and proceed to confirmation.</p> |
|  | <p>Device will display new time and date settings, cycling between year, month &amp; day, and time.</p> <p>YYYY→MM.DD→:HH:MM</p> <p>Press  key to return to normal weighing mode.</p>                                   |

## B. Device Setup

When the device is switched on, press and hold the  key for about 3 seconds, until the display shows the "SETUP", followed by "A.OFF" (first option in setting menu).

In device setup menu:



to toggle next menu option





to toggle previous menu option



to confirm selection / enter submenu





**Auto Power-Off:** Instruct device to shut off automatically after a certain period of time.


Press  to toggle between options (120 sec / 180 sec / 240 sec / 300 sec / off), and  to confirm selection.





**Buzzer/Beep:**

When function is turned on, beeping noise will be made when: indicator is turned on, keys are pressed, and weight is stable.

Press  to toggle between on/off, and  key to confirm selection.





**Hold Stop:** When Hold Stop is "on", Hold will deactivate after subject leaves measurement platform.

Press  to toggle between on/off, and  key to confirm selection.



LANGU

**Language:** Set thermal printer language

Press  to toggle between English, Italian and Polish. Press  key to confirm selection.



Font

**Font size:** Set thermal printer font size.

Press  to toggle between normal and double (larger). Press  key to confirm selection.



bluetooth

**Bluetooth (optional):** If device has Bluetooth module installed, Bluetooth function can be turned on or off.

Press  to toggle between on/off, and  to confirm selection.



Wi-Fi

**Wi-Fi (optional):** If device has Wi-Fi module installed, Wi-Fi function can be turned on or off.

Press  to toggle between on/off, and  to confirm selection.

Wi-Fi Setting

**Wi-Fi Setting (optional):** If device has Wi-Fi module installed, this option will appear.

Press  to toggle between on/off, and  to confirm selection.

## VI. Setup USB Connection to PC

For successful connection, PC hardware connected to device must be compatible with USB 2.0 or above. Operators should select a USB cable length that is most suitable to the operating environment.

1. Charder Smart Data Manager can be used to connect the device to a PC. The software program can be downloaded from the Charder website:

**[LINK URL]** <https://www.chardermedical.com/download.htm>

2. Connect USB cable to device indicator and PC. Follow installation instructions.

### Program Setup

1. After installation of Charder Smart Data Manager is complete, software will automatically search for COM port. Press **[Connect]**. Once connected, **[Connect]** button will change to **[Disconnect]**.

Charder Smart Data Manager COM [Connect]

|              |     |    |               |                |
|--------------|-----|----|---------------|----------------|
| Gross Weight | 0.0 | kg | First Name    | Enter          |
| Tare Weight  | 0.0 | kg | Last Name     | Enter          |
| Net Weight   | 0.0 | kg | Patient ID    | Enter          |
| Height       | 0.0 | cm | Date of Birth | 31 / 12 / 1990 |
| BMI          | 0.0 |    | Gender        | Male Female    |

Data

Please press "Connect"  
Update Time:  
Model:

## Conducting Measurement

1. Input subject's first name, last name, patient ID, date of birth (DD/MM/YYYY), gender, and height (for BMI calculation) into software if needed. Press **[Clear]** to clear all input.

**NOTE:** information can also be input after weight measurement.

The screenshot shows the 'chorder Smart Data Manager' interface. On the left, there are input fields for 'Gross Weight' (0.0 kg), 'Tare Weight' (0.0 kg), 'Net Weight' (0.0 kg), 'Height' (167.0 cm), 'BMI' (0.0), and a 'Data' section with 'Auto' and 'Manual' buttons. On the right, there are input fields for 'First Name' (Jane), 'Last Name' (Doe), 'Patient ID' (20190201), 'Date of Birth' (31 / 12 / 1965), and 'Gender' (Male/Female). A red box highlights the 'Height' field and the patient information fields. At the bottom, there are 'Collect', 'Clear', and 'Save as' buttons. A status message at the bottom left says 'Please press "Connect". Update Time: Model:'. The top right shows 'COM' and 'Connect' buttons.

2. Conduct measurement. If **[Auto]** is selected, results will be transmitted from device to software automatically and displayed on the left of screen. If **[Manual]** is selected, user must press "Collect".

The screenshot shows the 'chorder Smart Data Manager' interface after a measurement. The 'Gross Weight' is now 72.5 kg, 'Net Weight' is 72.5 kg, and 'BMI' is 26.0. The 'Height' field remains 167.0 cm. The patient information fields are the same. The 'Data' section now has 'Auto' selected. At the bottom left, there is a status message: 'Data updated. Update Time: 06/03/2020 11:40:00 Model:'. The top right shows 'COM' and 'Disconnect' buttons. The bottom buttons are 'Collect', 'Clear', and 'Save as'.

## Saving & Printing Results

1. Press **[Save as]** to save measurement results as .csv file on PC. Default file name is same as user ID. (ex: 20190201.csv) To track changes and multiple measurements for the same subject, we recommend not changing the default file name.

The screenshot shows the Chorder Smart Data Manager interface. It displays various patient data fields: Gross Weight (72.5 kg), Tare Weight (0.0 kg), Net Weight (72.5 kg), Height (167.0 cm), and BMI (26.0). Personal information includes First Name (Jane), Last Name (Doe), Patient ID (20190201), Date of Birth (31 / 12 / 1965), and Gender (Male). At the bottom, there are buttons for 'Collect', 'Clear', and 'Save as' (highlighted with a red box). A status bar at the bottom left indicates 'Data collected' and 'Update Time: 06/03/2020 11:40:00'.

## 2. Result example:

|   | A          | B          | C         | D          | E      | F          | G          | H          | I        | J   |
|---|------------|------------|-----------|------------|--------|------------|------------|------------|----------|-----|
| 1 | Patient ID | First Name | Last Name | Date of Bi | Gender | Gross Weig | Tare Weigt | Net Weight | Height   | BMI |
| 2 | 20190201   | Jane       | Doe       | 31/12/1965 | Male   | 72.4 kg    | 0.0 kg     | 72.4 kg    | 167.0 cm | 26  |
| 3 |            |            |           |            |        |            |            |            |          |     |
| 4 |            |            |           |            |        |            |            |            |          |     |
| 5 |            |            |           |            |        |            |            |            |          |     |


If previous results were saved in "20190201.csv", new results also need to be saved as "20190201.csv" (overwriting old file) in order to save multiple results for the same subject.

|   | A          | B          | C         | D          | E      | F          | G          | H          | I        | J   |
|---|------------|------------|-----------|------------|--------|------------|------------|------------|----------|-----|
| 1 | Patient ID | First Name | Last Name | Date of Bi | Gender | Gross Weig | Tare Weigt | Net Weight | Height   | BMI |
| 2 | 20190201   | Jane       | Doe       | 31/12/1965 | Male   | 72.4 kg    | 0.0 kg     | 72.4 kg    | 167.0 cm | 26  |
| 3 | 20190201   | Jane       | Doe       | 31/12/1965 | Male   | 75.2 kg    | 0.0 kg     | 75.2 kg    | 167.0 cm | 27  |
| 4 |            |            |           |            |        |            |            |            |          |     |

Results will be saved in chronological order of measurement.



3. Press the printer icon to print out result using a printer connected to the PC.

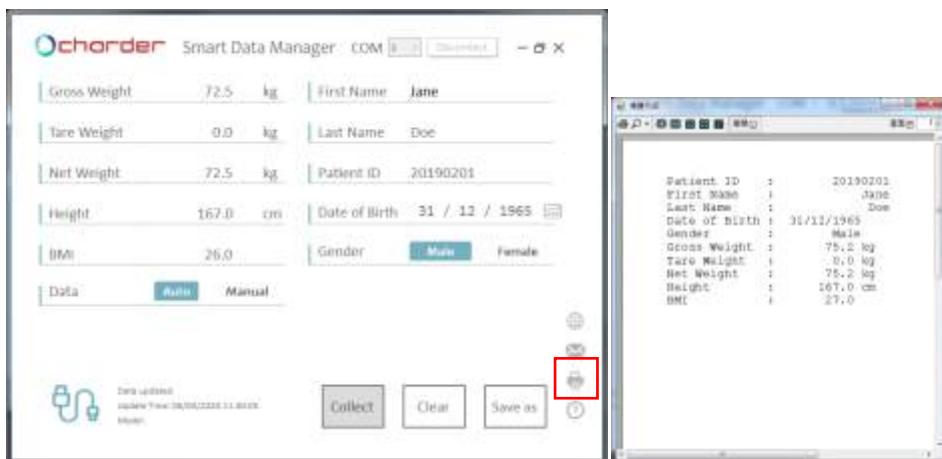

## VII. Wireless Connection

If the device has the wireless module installed, the indicator can transmit measurement results wirelessly. Please see Charder wireless software instructions for details.

## VIII. Troubleshooting

Before contacting your local Charder distributor for repair service, we recommend considering the following troubleshooting procedures:

### Self-inspection

#### 1. Device will not power on

- If battery power is depleted, replace with new batteries
- If batteries are not used, check if the power adapter is plugged into the device properly. Check if power adapter is plugged into mains properly

#### 2. Indicator showing "0000" ZERO SPAN out of range

- Interference due to factors such as RF disturbance or ground vibration. Relocate device to location without interference and try again
- Unstable platform feet - adjust wheel level according to bubble level indication and try again
- External objects interfering with measurement platform. Clear platform of objects and try again
- Device may not function properly on soft surfaces such as carpets or lawns. Relocate device to location with solid, stable floor
- If the steps above cannot resolve the problem, re-calibration may be required to correct weighing accuracy

#### 3. Connection failure for data transmission to PC or printer

- Ensure wires are connected correctly between indicator and PC or printer
- Ensure printer is supplied with power. Ensure PC software is set up properly as indicated in this manual

### Distributor support required

If the following errors occur, we recommend contacting your local Charder distributor for repair or replacement services:








#### 1. Device will not power on

- Faulty on/off key
- Broken or damaged wires causing short circuit or faulty connection
- Safety fuse burnout
- Faulty Adapter

## 2. Indicator damage

- Possible hardware defects include: uneven brightness in LCD screen, blurred text, smeared rainbow screen, incorrect decimal display
- Unable to save or read data
- Indicator shows "ERRL" after device is switched on
- Keys not responding
- Buzzer malfunction

### Error Messages

| Error Message  | Reason  | Action   |
|--|---|--|
|    | <b>Low battery warning</b><br>Voltage of battery is too low to operate device | Replace batteries, or plug in adapter  |
|    | <b>Overload</b><br>Total load exceeds device's maximum capacity               | Reduce weight on measurement platform and try again                            |
|    | <b>Counting Error (too high)</b><br>Signal from loadcells too high            | Error normally caused by faulty loadcell or wiring. Please contact distributor |
|    | <b>Counting Error (too low)</b><br>Signal from loadcells too low              | Error normally caused by faulty loadcell or wiring. Please contact distributor |
|   | Zero count over calibration zero range +10% while power on                    | Re-calibration required. Please contact distributor                            |
|  | Zero count under calibration zero range -10% while power on                   | Re-calibration required. Please contact distributor                            |
|  | <b>Program Error</b><br>Fault with device software                            | Error normally caused by faulty loadcell or wiring. Please contact distributor |


## IX. Product Specifications

|   |                   |   |                   |                   |
|---|-------------------|---|-------------------|-------------------|
| <b>Model</b>                                    |                   | <b>MS5410</b>   |                   |                   |
| <b>Display</b>                                  |                   | <b>DP3710</b>   |                   |                   |
| <b>Weight Measurement</b>                       | <b>Capacity</b>   | 150 kg x<br>50 g  | 250 kg x<br>100 g | 300 kg x<br>100 g |
|   | <b>Accuracy</b>   | ±1.5e   |                   |                   |
|   | <b>OIML</b>       | Class III   |                   |                   |
|   | <b>LCD Screen</b> | 1.0-inch LCD screen (5 1/2 digits)  |                   |                   |
| <b>Dimensions</b>                               | <b>Overall</b>    | 950(W) x 1040(D) x 640(H) mm  |                   |                   |
|   | <b>Seat</b>       | Height: 560mm<br>Width: 440 mm<br>Depth: 360 mm   |                   |                   |
|   | <b>Armrest</b>    | Height: 735 mm  |                   |                   |
| <b>Device Weight</b>                            |                   | 22.4 kg   |                   |                   |
| <b>Key Functions</b>                            |                   | On/Off, Zero, Print, BMI, Hold,<br>Pre-Tare, Tare, Clear, Enter, 0~9, M1-5<br>USB, Wireless Module (optional) |                   |                   |
| <b>Data Transmission</b>                        |                   | <b>NOTE:</b> Device should be connected to<br>network by qualified distributors only                          |                   |                   |
| <b>Power Supply</b>                             |                   | Rechargeable battery pack (optional)<br>or 6 AA batteries / Power adapter                                     |                   |                   |
| <b>Operation Temperature &amp;<br/>Humidity</b> |                   | 0°C~40°C    15% / 85% RH  |                   |                   |
| <b>Standard Accessories</b>                     |                   | User manual*1, Power Adapter*1<br>USB transfer cable*1  |                   |                   |
| <b>Optional Accessories</b>                     |                   | Thermal Printer   |                   |                   |



## Warning

The device is only compatible with the power adapters specified in the dashed block below.

| <b>AMP<br/>VOLTAGE</b> | <b>DRAWING NO.</b> | <b>CE APPROVED TYPE<br/>NO. / MODEL NO.</b> | <b>TYPE</b> | <b>Adapter<br/>plug</b>  |
|------------------------|--------------------|---|-------------|--|
| 12V 2A                 | AD-8058(AD-0521)   | UE24WU-120200SPA                            | US          |  |
|                        | AD-8057(AD-0520)   | UE24WV-120200SPA                            | EU          |  |
|                        | AD-8056(AD-0519)   | UE24WB-120200SPA                            | UK          |  |
|                        | AD-8074(AD-0534)   | UE24W4-120200SPAS                           | AU          |  |



# Notes

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---



---

---

---

## X. Declaration of Conformity

This product has been manufactured in accordance with the harmonized European standards, following the provisions of the below stated directives:

|   |  |
|---|--|
|  | 93/42/EEC as amended by 2007/47/EC<br>Medical Device Directive |
|   | 2014/31/EU<br>Non-automatic Weighing Instruments<br>Directive  |

*Please see separate document showing on sticker of device for above CE marking.*

Authorized EU Representative:



Manufactured by:  
Charder Electronic Co., Ltd.  
No.103, Guozhong Rd., Dali Dist.,  
Taichung City, 41262 Taiwan (R.O.C.)

CD-IN-00384 REV 001 04/2021